
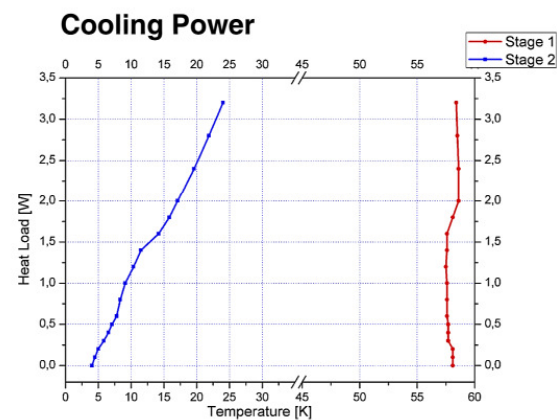



Closed-Cycle Systems

Two-Stage Pulse Tube Cryo-Cooler

- <4 K base temperature
- Custom cryostat setup for optical measurements
- Shielded sample room
- Custom, exchangeable sample holder
- optical access via windows and flanges
- optical tail piece exchangeable
- various custom options possible

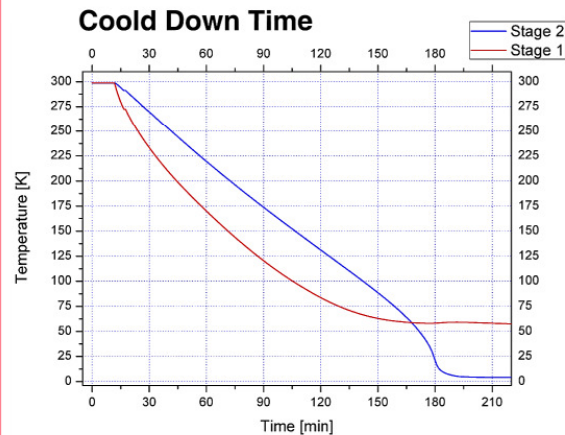

Additional heat load to 1. Stage 1W

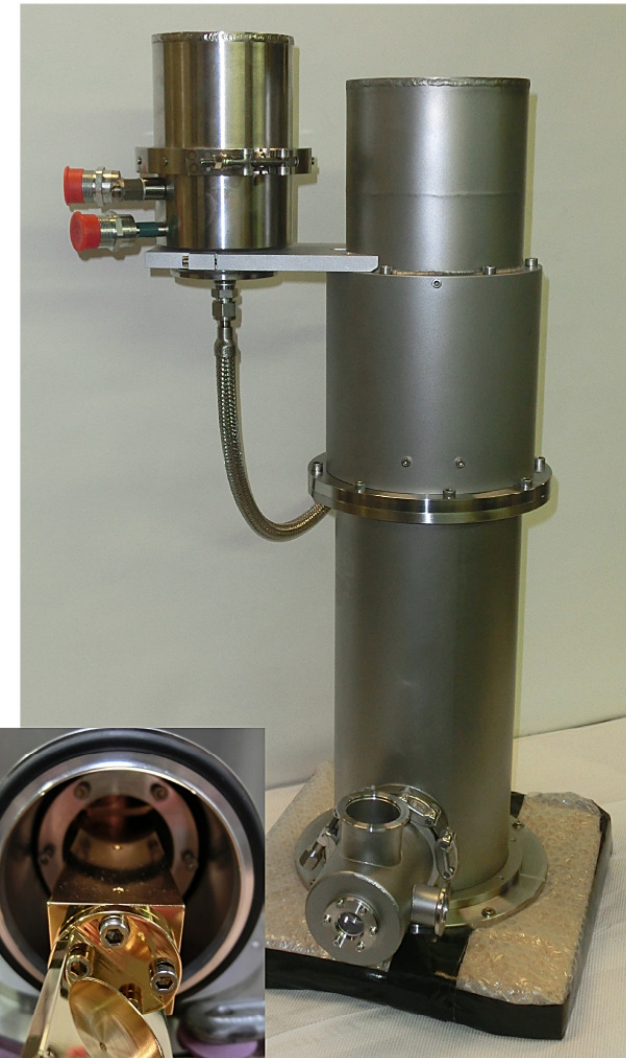

exchangeable
sample holder